

# Spirodoc®

**One Touch Laboratory for respiratory analysis**  
**two functional modes: doctor and patient**



 **reddot design award**  
winner 2010 - 2011



**Spirometer**  
with "Touch Screen"  
display



**Pulse Oximeter**  
"intelligent" with  
on screen results



**Six Minute Walk Test**  
three phase print-out:  
baseline, walk and  
recovery



**Questionnaire**  
for home care  
symptom control  
recovery

# Spirodoc®



Spirometry menu in "Doctor mode"




## Complete Spirometer ATS/ERS compliant

### Specialist-level analysis, screening and home care monitoring

The New Spirodoc® has been developed with great attention both to design and technology, with various operation modes: "advanced" parameters for the specialist, "reduced" set of parameters for screening as well as a "simplified" version for Home Care operation.


FVC, VC, IVC, MVV, PRE-POST.  
Precise spirometry interpretation including post bronchodilator.  
All tests are automatically memorized.  
Automatic BTPS conversion.  
Memory capacity: 10.000 tests.  
Wide selection of predicted values.

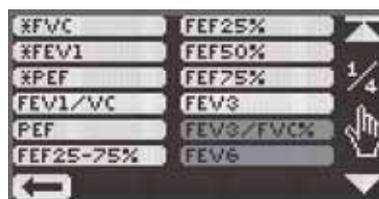

Choice of spirometric parameters



Patient data entry

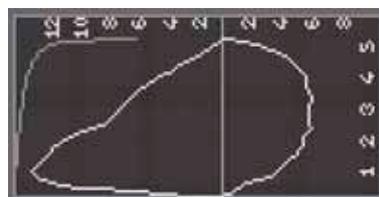

Flow/Volume and Volume/Time curves

### FlowMIR®: disposable turbine



Spirometry requires maximum accuracy and hygiene. FlowMir® is the answer to both requirements. Each turbine is calibrated with a computerized system and it is packaged individually. After patient testing both the turbine and mouthpiece are thrown away. In this way 100% hygiene can be guaranteed.

### Option available: reusable turbine



The accuracy and the precision of the reusable turbine remains unchanged even over time.

**SPIRO DETACHABLE HEAD**



**Spirometry option.**

Flow and volume measurements made by digital turbine system for a reliable result.



Paediatric and adult finger probe



Neonatal flex probe

# Intelligent Pulse Oximeter with on-screen results

## Six Minute Walking Test

Simple, clear SpO2 and Pulse Rate measurements with plethysmographic curve.

A single six-minute walk test can be made and all results are shown directly on the display.

Innovative and essential in pneumology, cardiology and rehabilitation etc.



Belt with silicon holder (option).



Plethysmographic Curve



Oximetry Menu



Patient Data Entry

## Day and night



Spirodoc® carries out a sleep desaturation study and memorizes events.



Parameter Choice

# One Touch Laboratory for respiratory analysis



## Ideal for rehabilitation, telemedicine and clinical trials

**Spirodoc® has all of these features.**

Spirodoc® conforms to the  
**EU guidelines for Telemedicine and COPD:**

- respiratory function (**spirometer**)
- desaturation analysis (**pulse oximeter**)
- daily questionnaire (**symptoms**)
- physical activity (**6MWT**).

**Home-care symptoms diary**

Fast on-screen symptoms entry.  
Complete touch screen  
with settable questions and  
automatic answer recording  
for homecare patient use  
(**eDiary**).

### Respiratory rehabilitation and Activity Monitoring



According to the latest  
ATS COPD Guidelines,  
it is fundamental that, for  
patients with respiratory  
diseases, the level of exercise  
during the rehabilitation phase  
can be studied.

### Telemedicine Anywhere




WinspiroPRO is a unique featured PC software, which comes standard with all MIR spirometers and oximeters.

The latest version provides an innovative user interface.



Summary of all tests carried out

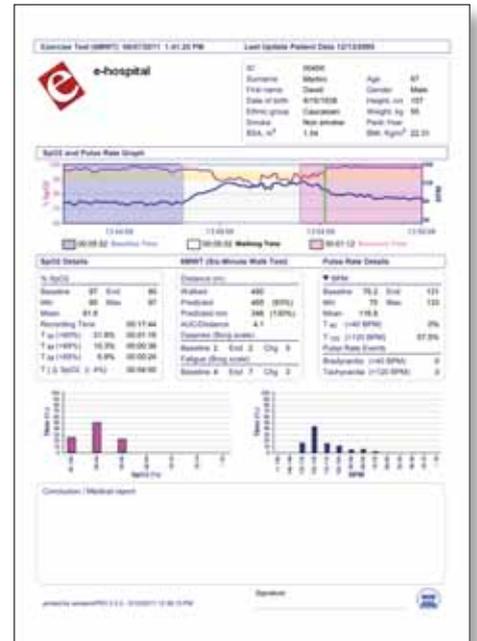

Printout of the 6 minute walking test: baseline, walk, recovery

## Comprehensive patient records

Dynamic management of all data and graphs including SpO2 measurements during the corresponding test (6MWT, Sleep, Stress Test...).

# WinspiroPRO now available with HL7 interface

## High performance PC software for spirometry and oximetry

All results can be rapidly printed.

All tests memorised in Spirodoc® are automatically downloaded into winspiroPRO and a patient data card is automatically created with a preview of the spirometry curve.

The spirometry incentive routine, patented by MIR, allows the user to select the patient's favourite image in order to get maximum compliance.

WinspiroPRO can easily be connected to a database, EPR, hospital or occupational health system. Special edition with HL7 interface is available on request.


This software also gives trend graphs of any parameter, ideal for clinical trials and telemedicine.

All tests and curves for every patient in the memory can be reviewed on a single page and the results, including oximetry tests, can be compared.



Printout of sleep oximetry with desaturation analysis

# Spirodoc®

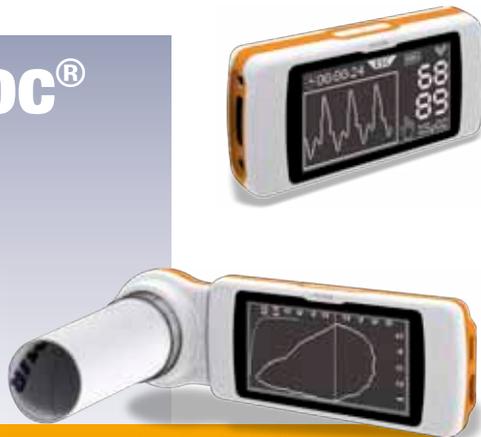

## Spirometer technical specifications

Flow sensor: bi-directional digital turbine  
 Flow range  $\pm 16\text{L/s}$   
 Volume accuracy:  $\pm 3\%$  o 50mL, whichever is greater  
 Flow accuracy:  $\pm 5\%$  o 200mL/s, whichever is greater  
 Dynamic resistance at 12L/s:  $< 0.5\text{cmH}_2\text{O/L/s}$   
 Temperature sensor: semiconductor (0-45°C)

## Spirometer measured parameters

FVC, FEV1, FEV1/FVC%, FEV3, FEV3/FVC%, FEV6, FEV1/FEV6%, PEF, FEF25%, FEF50%, FEF75%, FEF25%-75%, FET, Estimated Lung Age, Extr. Vol., FIVC, FIV1, FIV1/FIVC%, PIF, VC, IVC, IC, ERV, FEV1/VC%, VT, VE, Rf, ti, te, ti/t-tot, VT/ti, MVV measured, MVV calculated



## Central unit technical specifications

Display: LCD Backlit Touch screen Display:  
 Resolution: 128x64 pixels  
 Power supply: Lithium ion 3.7V, 1100mA rechargeable battery with 30 hours measurement back-up  
 Data transmission: USB 2.0 (Bluetooth® optional)  
 Dimensions and weight:  
 central unit 101x48x16mm, 99g  
 removable turbine head: 46x47x24mm, 17g  
 Battery charger (optional): 100VAC - 240VAC, 50Hz-60Hz  
 output 5VDC, 500mA, micro USB type B

## Pulse-oximeter technical specifications

SpO2 range: 0-100%  
 SpO2 accuracy:  $\pm 2\%$  (50-100% SpO2)  
 Pulse rate range: 20-254BPM  
 Heart rate accuracy:  $\pm 2\text{BPM}$  or 2%, whichever is greater

## Pulse-oximeter measured parameters (standard)

SpO2 [Baseline, Min, Max, Mean], Pulse rate [Baseline, Min, Max, Mean], T90% [SpO2<90%], T89% [SpO2<89%], T88% [SpO2<88%], T5% [ $\Delta\text{SpO}_2 > 5\%$ ],  $\Delta\text{Index}$  [12s], SpO2 Events, Pulse rate events [Bradycardia, Tachycardia], Recording time, Analysis time

## Sleep analysis (specific parameters)

SpO2 Events, Desaturation index (ODI), Desaturation [Mean Value, Mean duration, Longest duration, Nadir Peak],  $\Delta\text{SpO}_2$  [Min Drop, Max Drop], Total Pulse Variations, Pulse Rate Index, NOD89% [SpO2<89%; >5min], NOD4% [SpO2 Basale-4%; >5min], NOD90% [SpO2<90%; Nadir<86%; >5min]

## 6MWT (6 Minute Walk Test specific parameters)

Distance walked, Predicted distance [Min, Standard],  $\text{T}\Delta 2\%$  [SpO2 $\geq 2\%$ ],  $\text{T}\Delta 4\%$  [ $\Delta\text{SpO}_2 \geq 4\%$ ], Time [Rest, Walking, Recovery], Desaturation Area/Distance

**Optional data entry:** Borg Dyspnea [Baseline, End, Change], Borg Fatigue [Baseline, End, Change], Arterial blood pressure [Systolic, Diastolic], Oxygen administered